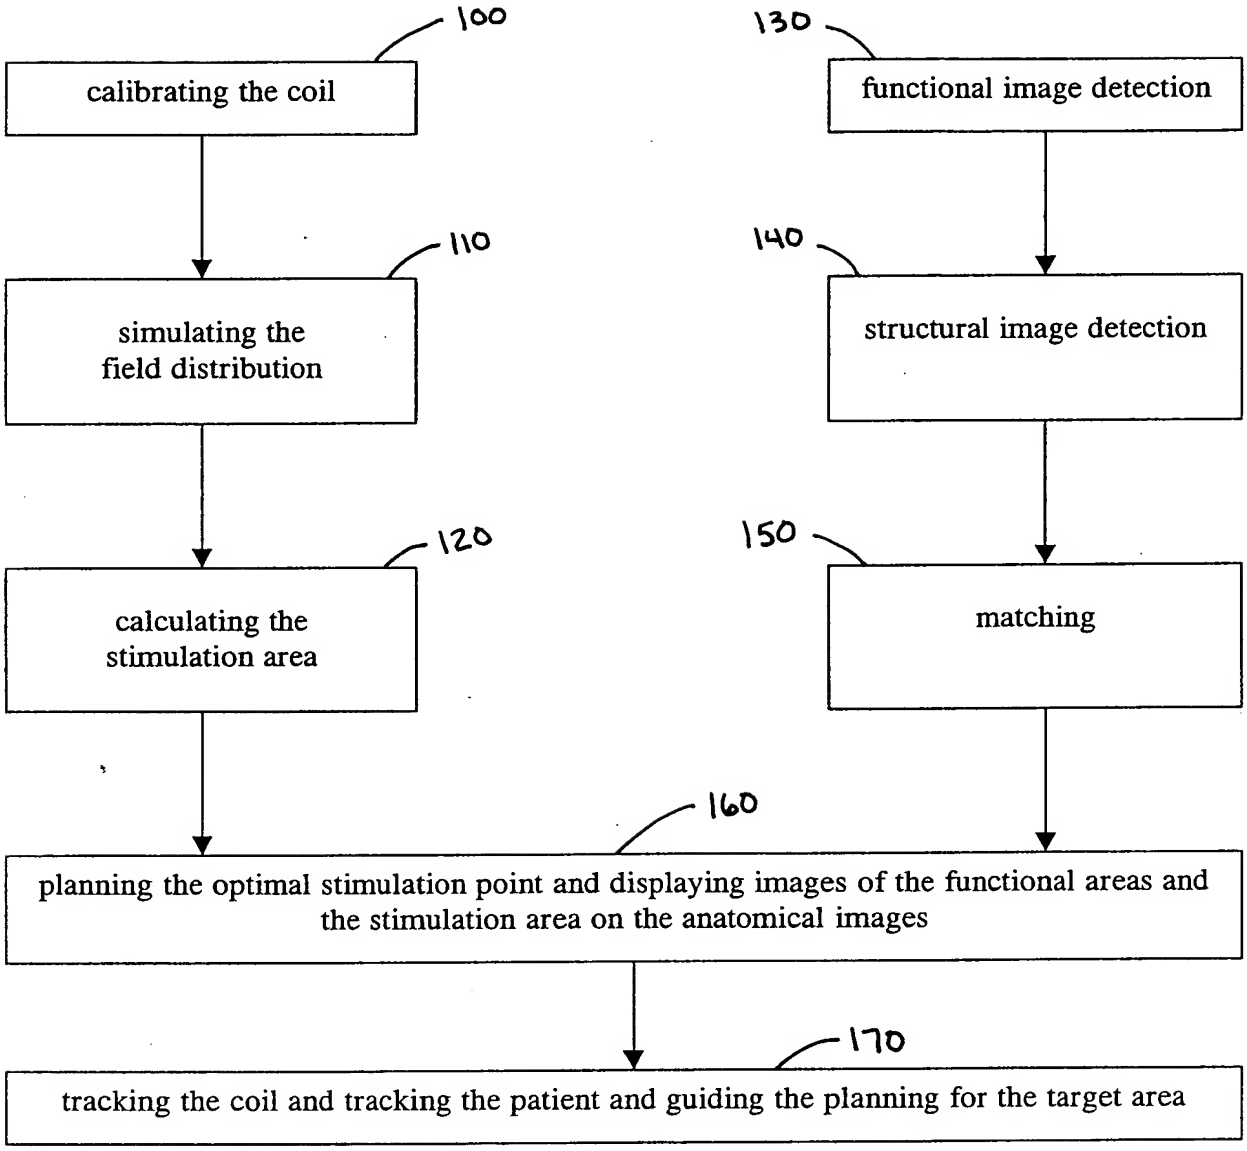
100
calibrating the coil
110
simulating the field distribution
120
calculating the stimulation area
130
functional image detection
140
structural image detection
150
matching
160
planning the optimal stimulation point and displaying images of the functional areas and the stimulation area on the anatomical images
170
tracking the coil and tracking the patient and guiding the planning for the target area

FIG. 1